

VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

JUL 07 2009

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	<u>130125</u>
Name		<u>Gary Tellep</u>	ID# <u>2281</u> Date <u>4/10/09</u>
A	Agency	<u>AST/Fairbanks</u>	Phone # _____
Instrument Location		<u>AST/Fairbanks</u>	_____
Alco S/N		<u>X172978</u>	Target Value <u>0.081</u> High Pressure _____
B	Alco Test Values		<u>0.077</u> 1 st Alco <u>0.079</u> 2 nd Alco
Signature		<u>Gary Tellep</u>	<u>COB</u> <u>7/13/09</u>
(OVER)			

(Do Not write in the area below)


I, Nita J. Bolz, after being first duly sworn, depose and state as follows:

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.

Nita J. Bolz
Nita J. Bolz
Scientific Director
State Breath Alcohol Program

Subscribed and sworn before me this 13th day of July, 2009.

Carolyn M. Noland (Notary Seal Stamp)
Carolyn M. Noland
Notary Public, State of Alaska
Commission Expires with Office



VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N


130125 ✓

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

NONDRINKING SUBJECT TEST

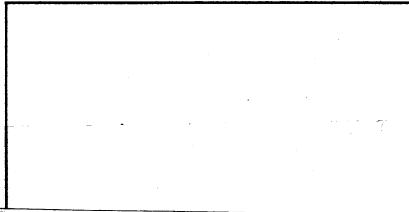

Breath Test Record

Serial Number 130125 Model DataMaster
Location FBK0 AST/Fairbanks

CD #1301

Subject Information


Last Name Verification Of Cal O.L. # N
First Name N

Operator Information


Operator Name Tellep Gary J Case N
Operator # 2281 Department FBK0

Test Results

Alco Target .081 Alco Serial X172978
Nominal 0.078 Barometer 29.10 Test Type V
Dry Gas 1 0.077 Time: 01:01:40 Test Date 04/10/2009
Subject Alcohol 0.000 Time: 01:02:56 Test Time 01:00:18
Dry Gas 2 0.079 Time: 01:03:59 Report Y

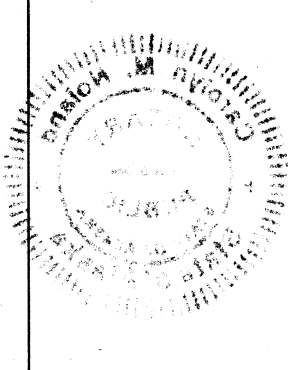

DIAGNOSTIC CHECK

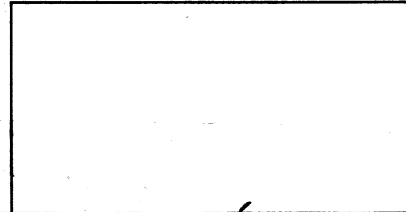

Diagnostic Test Record

Serial Number 130125 Model DataMaster
Location FBK0 AST/Fairbanks

Diagnostic Test Results

Test Date 04/10/2009 Computer Okay
Test Time 01:06:00 Program Okay
Software Date 02/20/2001
Sample Chamber (C) 49
Breath Tube (C) 40
Barometer (in) 29.10
Flow Detector Okay
High Speed Pump Okay
Detector Okay
Filter Okay
Quartz Okay
Calibration Okay

